

		Units
 +5V	6	A
Output Regulation	0.05	%

Inputs, Outputs, and Controls

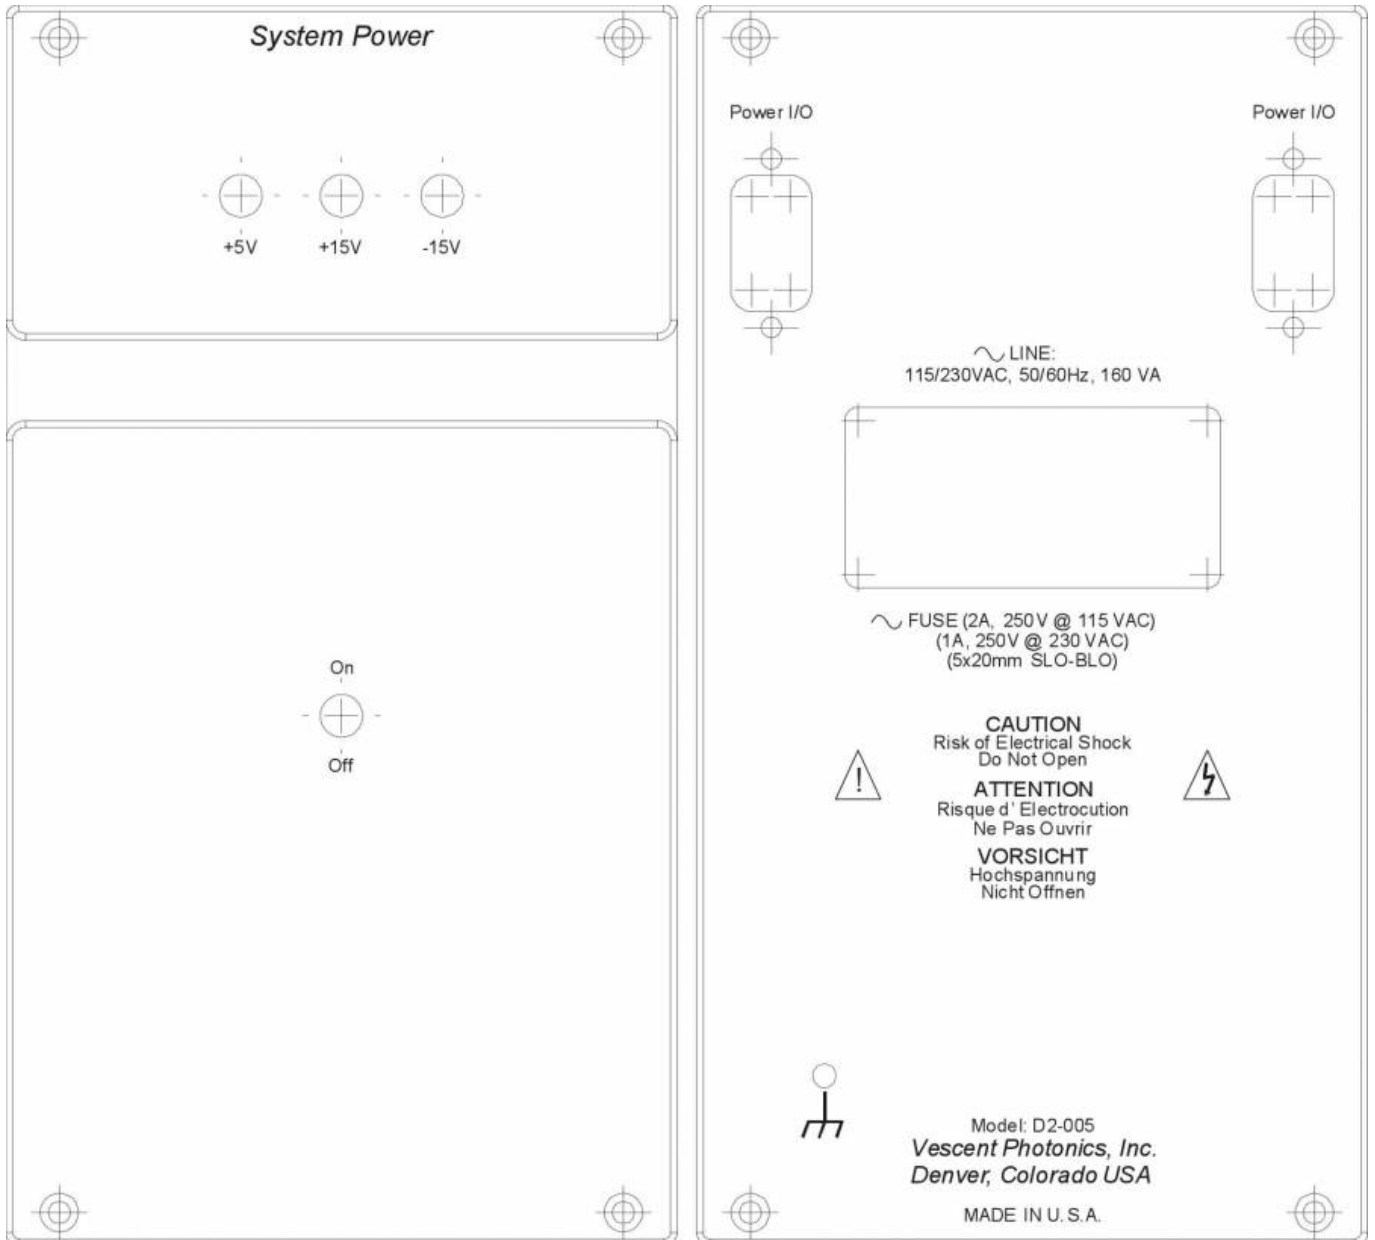


Fig. 1: Schematic drawing of the front and back panels of the D2-005

Monitor Section

The monitor section contains three blue status LEDs indicating proper voltage on the +15,-15, and 5V power lines. If there is a voltage sag on any of the power lines, the blue status LED will turn off.

Back panel I/O

Power I/O (9-pin D-sub)





Always turn off the D2-005, make connections to the device, and then re-energize the D2-005. Never connect this D2-005 Power Supply to a device when it is switched on and supplying power.



If you are considering using an Uninterruptible Power Supply (UPS) to guarantee operation of your Vescent products through a brown out or black out, great care should be taken in choosing the model. Lower cost models tend to produce modified square wave voltage profiles. The high-frequency components of such a voltage profile may interact poorly with the D2-005 (and down-stream active Vescent modules). If you do choose to use a UPS, select a model that will provide a sine wave voltage profile without higher harmonic components to avoid potential damage to your high-value equipment.

The power to each electronics module is through a 9-pin D-sub connector through a power bridge unit. The unit can also be powered through any serial cable with 9-pin D-sub connectors, which is convenient when the unit must be taken out of line for access to the side panels. The pin outs are shown in the following figure:

D-Sub Power Pin Out
(female connector drawn)

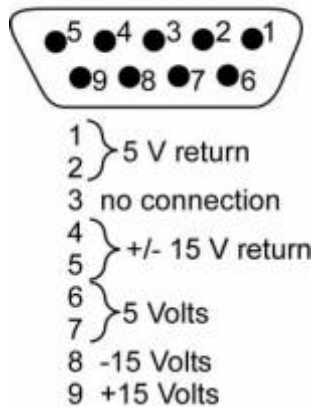

From:

<https://www.vescent.com/manuals/> - **Product Manuals**

Permanent link:

https://www.vescent.com/manuals/doku.php?id=d2:power_supply

Last update: **2018/10/15 13:11**

