

# Power Supply

Model No. D2-005

Document Revision: 1

Document Last Updated on 2022/08/23 20:14

Please read [Limited Warranty](#) and [General Warnings and Cautions](#) prior to operating the D2-005.

Link to [D2-005 Power Supply web page](#)

For technical assistance, please contact Vescent at:  
14998 W. 6th St.  
Golden, CO 80401  
USA

or

info [at] vescent [dot] com



## Description

The Power Supply is a quiet, linear power supply providing +/-15V and 5V. It is in a separate box to isolate 60 Hz and EM interference. One power supply can power two complete laser systems, or four electronics modules.

## Warnings

This manual must be consulted in all cases where the Caution symbol is marked, in order to find out the nature of the potential hazards and any actions which have to be taken to avoid them.

**Caution: Risk of Electrical Shock Do Not Open** – The D2-005 contains high voltage components and should never be opened in any circumstance except by trained Vescent personnel.



There are no serviceable parts in the D2-005. Only Vescent is authorized to service this product.



Nothing must obstruct airflow from the top panel vent. Never place anything on top of the D2-005.

## Purchase Includes

- D2-005 Power Supply
- VPN00464 Power Cord

## Absolute Maximum Ratings

Note: All modules designed to be operated in laboratory environment with filtered air. There are no known altitude restrictions on the D2-005.

Parameter	Rating
Environmental Temperature	>15°C and <30°C
Environmental Humidity	<60%
Environmental Dew Points	<15°C

## Specifications

		Units
Current Limit		
+15V	1.5	A
-15V	1.5	A
+5V	6	A
Output Regulation	0.05	%
Input Voltages	100±10, 120±10, 230±10	V
Input Frequency	50, 60	Hz
Power Rating	160	VA

## Inputs, Outputs, and Controls

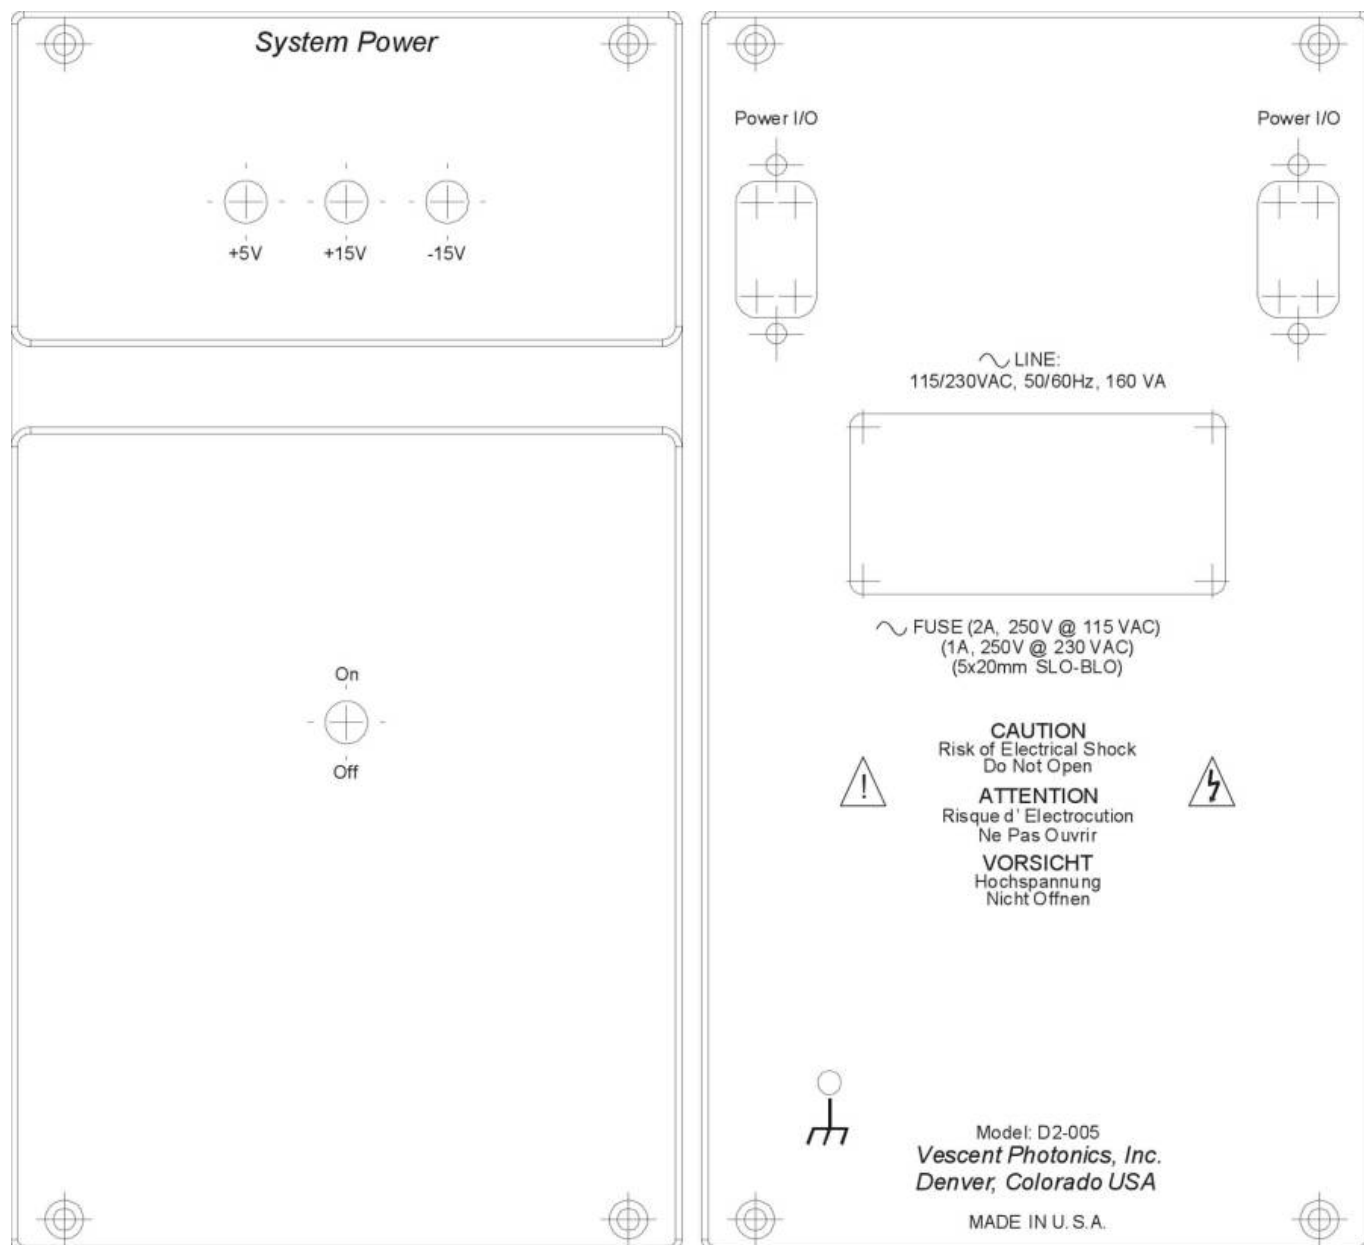


Fig. 1: Schematic drawing of the front and back panels of the D2-005

## Monitor Section

The monitor section contains three blue status LEDs indicating proper voltage on the +15,-15, and 5V power lines. If there is a voltage sag on any of the power lines, the blue status LED will turn off.

## Back panel I/O

### Power I/O (9-pin D-sub)




Always turn off the D2-005, make connections to the device, and then re-energize the D2-005. Never connect this D2-005 Power Supply to a device when it is switched on and supplying power.



If you are considering using an Uninterruptible Power Supply (UPS) to guarantee operation of your Vescent products through a brown out or black out, great care should be taken in choosing the model. Lower cost models tend to produce modified square wave voltage profiles. The high-frequency components of such a voltage profile may interact poorly with the D2-005 (and down-stream active Vescent modules). If you do choose to use a UPS, select a model that will provide a sine wave voltage profile without higher harmonic components to avoid potential damage to your high-value equipment.

Power is supplied to the D2-005 via a standard C13 to Type-B power cord. The power to each electronics module is through a 9-pin D-sub connector through a power bridge unit. The unit can also be powered through any serial cable with 9-pin D-sub connectors, which is convenient when the unit must be taken out of line for access to the side panels. The pin outs are shown in the following figure:

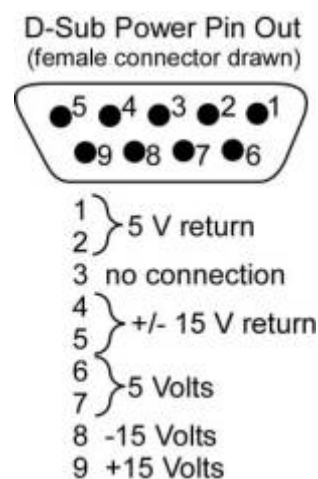

While it is infrequent, the D2-005 may occasionally radiate noise from the side of its chassis onto nearby electronics. This only occurs in some system configurations, and will appear as a signal at the frequency of your mains electricity (typically either 50 Hz or 60 Hz). This noise can easily be removed by moving the D2-005 at least 18 inches (45cm) away from other electronics, rotating it 90° such that the sides of the D2-005 face away, or by moving the entire power supply to a different shelf. To accommodate this, all D2-005's are shipped with a 5' DB9 cable as of January 1, 2022.

From:  
<https://www.vescent.com/manuals/> - **Product Manuals**

Permanent link:  
[https://www.vescent.com/manuals/doku.php?id=d2:power\\_supply&rev=1661285677](https://www.vescent.com/manuals/doku.php?id=d2:power_supply&rev=1661285677)

Last update: **2022/08/23 20:14**

